

इंटरनेट

मानक

Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

“जानने का अधिकार, जीने का अधिकार”

Mazdoor Kisan Shakti Sangathan

“The Right to Information, The Right to Live”

“पुराने को छोड़ नये के तरफ”

Jawaharlal Nehru

“Step Out From the Old to the New”

IS 4149 (1967): Post-mortem Rubber Gloves [PCD 13: Rubber and Rubber Products]



“ज्ञान से एक नये भारत का निर्माण”

Satyanarayan Gangaram Pitroda

“Invent a New India Using Knowledge”



“ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है”

Bhartrhari—Nitiśatakam

“Knowledge is such a treasure which cannot be stolen”

BLANK PAGE



IS : 4149 - 1967

(Reaffirmed 2012)

Indian Standard
SPECIFICATION FOR
POST-MORTEM RUBBER GLOVES

(Second Reprint APRIL 1990)

UDC 615.479.47:616-091.5

© Copyright 1967

BUREAU OF INDIAN STANDARDS
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG
NEW DELHI 110002

Indian Standard

SPECIFICATION FOR

POST-MORTEM RUBBER GLOVES

Rubber Products Sectional Committee, CDC 6

Chairman

DR D. BANERJEE

Representing

National Rubber Manufacturers Ltd, Calcutta; and
Association of Rubber Manufacturers in India,
Calcutta

Members

SHRI P. K. BOSE	The Dunlop Rubber Co (India) Ltd, Calcutta
SHRI S. MUKHERJEE (<i>Alternate</i>)	National Test House Calcutta; and Directorate General of Supplies & Disposals (Ministry of Supply, Technical Development & Materials Planning)
SHRI R. C. DASGUPTA	
SHRI S. P. MULLICK (<i>Alternate</i>)	
SHRI S. L. GANDHI	Ministry of Defence (DGI)
SHRI S. C. GANGULI	Ministry of Defence (R & D)
SHRI B. K. DATTA GUPTA (<i>Alternate</i>)	
SHRI K. K. GANGULY	Ministry of Defence (R & D)
SHRI LALIT MOHAN JAMNADAS	The Cosmos India Rubber Works Private Ltd, Bombay
SHRI SHAM SUNDAR AZAD (<i>Alternate</i>)	
SHRI S. R. KOCHHAR	Inspection Wing, Directorate General of Supplies & Disposals (Ministry of Supply, Technical Development & Materials Planning)
SHRI K. M. KUKERJA	Hindustan Steel Ltd, Ranchi
SHRI G. C. JAIN (<i>Alternate</i>)	
SHRI R. C. KURILLAYA	Indian Oil Corporation Ltd (Marketing Division), Bombay
DR K. N. MODAK	Indian Rubber Manufacturers Research Association, Bombay; and All India Automobile & Ancillary Industries Association, Bombay
DR D. K. ROYCHAUDHURI	I. C. I. (India) Private Ltd, Calcutta
DR B. B. BHATIA (<i>Alternate</i>)	
DR A. SEETHARAMIAH	Directorate General of Technical Development (Ministry of Supply, Technical Development & Materials Planning)
DR N. V. C. RAO (<i>Alternate</i>)	
SHRI K. R. SENGUPTA	Indian Rubber Industries Association, Bombay
SHRI B. BASU (<i>Alternate</i>)	
SHRI M. C. SINGHAL	Railway Board (Ministry of Railways)

(Continued on page 2)

BUREAU OF INDIAN STANDARDS
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG
NEW DELHI 110002

(Continued from page 1)

Members

DR N. H. SIVARAMAKRISHNAN
DR SADGOPAL,
Director (Chem)

Representing

Rubber Board, Kottayam
Director General, ISI (*Ex-officio Member*)

Secretary

SHRI N. R. SRINIVASAN
Assistant Director (Chem), ISI

Medical Rubber Goods Subcommittee, CDC 6:7

Convener

DR UMA SHANKAR

Swastik Rubber Products Ltd, Poona

Members

SHRI V. D. PENDSE (*Alternate to*
Dr Uma Shankar)

DR S. R. AGRAWAL

Johnson & Johnson of India Ltd, Bombay

SHRI V. N. NAGARSENKAR (*Alternate*)

DR B. B. BHATIA

I. C. I. (India) Private Ltd, Calcutta

SHRI S. K. BORKAR

Directorate General of Health Services (Ministry of
Health)

SHRI D. BOSE

Bengal Waterproof Works (1940) Ltd, Calcutta

SHRI A. BOSE (*Alternate*)

SHRI R. C. DASGUPTA

Directorate General of Supplies & Disposals
(Ministry of Supply, Technical Development &
Materials Planning)

SHRI S. P. MULLICK (*Alternate*)

EXECUTIVE SECRETARY

Family Planning Association of India, Bombay

SHRI S. L. GANDHI

Ministry of Defence (DGI)

MAJ K. D. KAPOOR

Directorate General of Armed Forces Medical Ser-
vices (Ministry of Defence)

SHRI S. V. LATHIA

Industrial Supplies Corporation, Bombay

SHRI S. C. MOHAN

Small Scale Latex Products Association, New Delhi

SHRI R. K. DHAWAN (*Alternate*)

SHRI S. W. NEWMAN

London Rubber Co (India) Ltd, Madras

SHRI S. A. PASHA (*Alternate*)

SHRI M. G. PANDIT

Directorate General of Health Services (Ministry of
Health)

DEPUTY ASSISTANT DIRECTOR

GENERAL OF HEALTH SERVICES (*Alternate*)

SHRI MANUBHAI M. PATEL

Rubbrex Industries Private Ltd, Bombay

SHRI K. G. SHAH (*Alternate*)

SHRI W. S. RAJADHYAKSHA

Associated Rubber Industries Ltd, Bhavnagar

SHRI M. N. PATHAK (*Alternate*)

Indian Standard

SPECIFICATION FOR

POST-MORTEM RUBBER GLOVES

0. FOREWORD

0.1 This Indian Standard was adopted by the Indian Standards Institution on 25 April 1967, after the draft finalized by the Rubber Products Sectional Committee had been approved by the Chemical Division Council.

0.2 Rubber post-mortem gloves are manufactured by solution-dip and latex-dip processes. They may also be built up from sheet rubbers. In the formulation of this standard due weightage has been given to all such manufacturing practices prevailing in this country.

0.3 The dimensions prescribed for gloves in this standard correspond to the popularly known size 8 in rationalized metric values.

0.4 In the preparation of this standard, assistance has been derived from B.S. 1844 : 1952 'Rubber post-mortem gloves' issued by the British Standards Institution.

0.5 This standard contains clauses 3.4, 3.8.2 and 5.1 which call for agreement between the purchaser and the supplier.

0.6 For the purpose of deciding whether a particular requirement of this standard is complied with, the final value, observed or calculated, expressing the result of a test or analysis, shall be rounded off in accordance with IS : 2-1960*. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1. SCOPE

1.1 This standard prescribes the requirements and methods of sampling and test for gloves made from natural or synthetic rubber for use in post-mortem surgical work.

*Rules for rounding off numerical values (revised).

2. TYPES

2.1 This specification covers the following three types of gloves known after their process of manufacture:

- Type A Solution-dipped gloves,
- Type B Latex-dipped gloves, and
- Type C Hand-made gloves.

3. REQUIREMENTS

3.1 All types of post-mortem gloves shall be made from natural or synthetic rubber or a blend of both by hot vulcanization.

3.2 Hand-made gloves shall be made by butt or skive jointing from calendered sheets. All the joints shall be reinforced with strips of rubber sheet.

3.3 No ingredient, which is injurious or cause irritation to living human skin coming in contact with the finished gloves, shall be included.

3.4 The gloves shall have rough or smooth finish as agreed to between the purchaser and the supplier. The wrists shall have edges rolled up or cut and reinforced rubber strips.

3.5 The gloves shall conform to the dimensions given in Table I and as shown in Fig. 1 which shows a right hand post-mortem glove.

TABLE 1 DIMENSIONS OF POST-MORTEM RUBBER GLOVES

All dimensions in millimetres.		
DESCRIPTION	DIMENSION	TOLERANCE
Perimeter at <i>AA</i>	210	±3
Perimeter at <i>BB</i>	185	
Perimeter at <i>CC</i>	240	
Perimeter at <i>DD</i>	205	
Circumference at <i>E</i>	60	±2
Circumference at <i>F</i>	63	
Circumference at <i>G</i>	65	
Circumference at <i>H</i>	70	
Length at <i>J</i>	61	
Length at <i>K</i>	120	±2
Length at <i>L & N</i>	72	
Length at <i>M</i>	82	
Length at <i>O</i>	62	
Length at <i>P</i>	280	±3
Length at <i>Q</i>	195	
Length at <i>R</i>	9	±1

NOTE — All the dimensions given here are outside dimensions. Circumference at *E*, *F*, *G* and *H* is to be measured at a point 5 mm less than the length of the respective finger as measured from the tip.

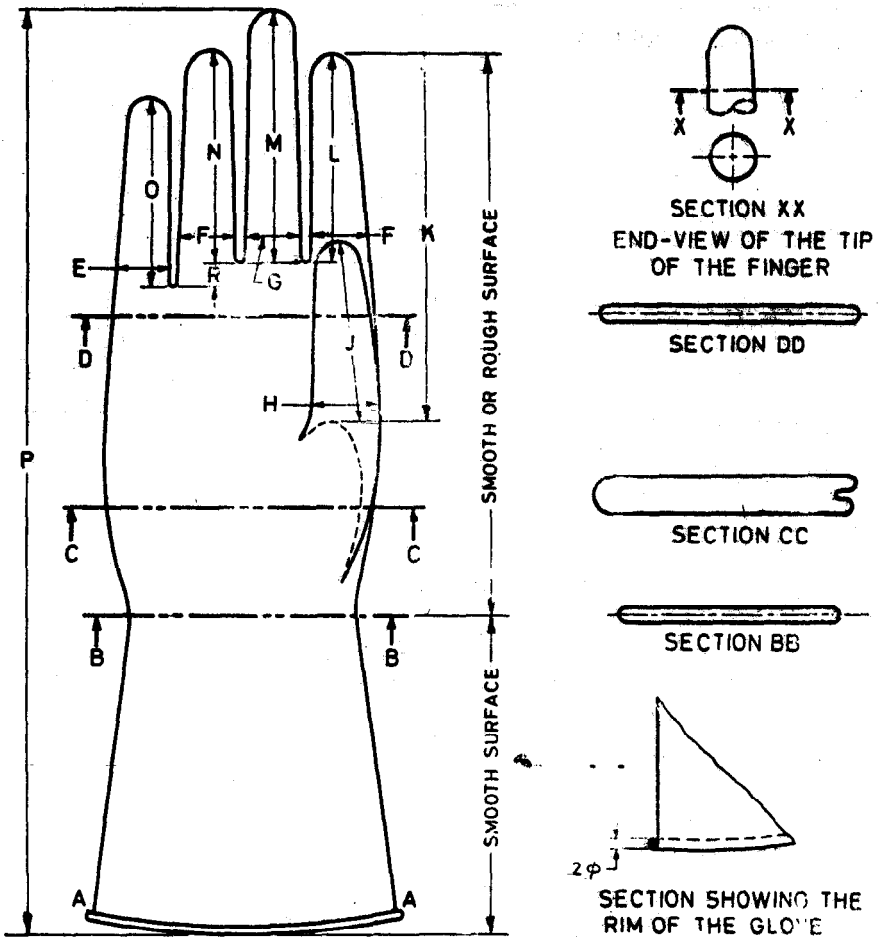


FIG. 1 RIGHT HAND POST-MORTEM RUBBER GLOVE

3.6 Physical Properties of Rubber

3.6.1 Tensile Strength and Elongation at Break — Requirements for tensile strength and elongation at break for the samples tested before heat-treatment shall be in accordance with the requirements given in Table 2.

TABLE 2 TENSILE STRENGTH AND ELONGATION AT BREAK

(Clause 3.6.1)

TYPE OF GLOVE	BEFORE HEAT-TREATMENT	
	Tensile Strength, Min kg/cm ²	Elongation at Break, Min percent
(1)	(2)	(3)
A	105	500
B	140	600
C	105	500

3.6.2 Tension Set — Test pieces shall not show tension set exceeding 10 percent when tested according to the method prescribed in 7.3.

3.6.3 Requirements for the samples tested after heat-treatment shall not vary by more than +0, - 20 percent for tensile strength and +0, -20 percent for elongation at break from the corresponding values given in Table 2 (see 3.6.1).

3.7 Aqueous extract of rubber of the gloves shall not be acidic to methyl orange or alkaline to phenolphthalein when tested according to the method prescribed in 7.4.

3.8 Workmanship and Finish — The gloves shall be free from perforations and other imperfections. They shall not show any sign of porosity.

3.8.1 The gloves shall not crumple or take crease.

3.8.2 The colour of the gloves shall be as agreed to between the purchaser and the supplier.

3.8.2.1 The recommended colours are pinkish red or black.

4. MARKING

4.1 Each glove shall be legibly marked with the following particulars:

- Manufacturer's name or trade-mark, if any;
- Size of glove;
- Month and year of manufacture; and
- Type.

4.1.1 Post-mortem rubber gloves may also be marked with the ISI Certification Mark.

NOTE — The use of the ISI Certification Mark is governed by the provisions of the Indian Standards Institution (Certification Marks) Act and the Rules and Regulations made thereunder. The ISI Mark on products covered by an Indian Standard conveys the assurance that they have been produced to comply with the requirements of that standard under a well-defined system of inspection, testing and quality control which is devised and supervised by ISI and operated by the producer. ISI marked products are also continuously checked by ISI for conformity to that standard as a further safeguard. Details of conditions under which a licence for the use of the ISI Certification Mark may be granted to manufacturers or processors, may be obtained from the Indian Standards Institution.

5. PACKING

5.1 The material may be packed in polyethylene bags or as agreed to between the purchaser and the supplier.

6. SAMPLING AND CRITERIA FOR CONFORMITY

6.1 For the purpose of ascertaining the conformity of the gloves in a consignment to this specification, the scale of sampling and the criteria for conformity shall be as prescribed in Appendix A.

7. TEST METHODS

7.1 Tensile Strength and Elongation — Determine tensile strength and elongation at break in accordance with the method prescribed in IS : 3400 (Part I)-1965*.

7.2 Heat-Treatment Test — Wrap a suitable portion of the glove or suitable test pieces cut from a glove in a surgical gauze in such a manner that all the rubber surfaces are separated from one another and are subjected to treatment in saturated steam at a temperature of 115° to 120°C for a period of 20 minutes. Make sure to remove all the air from the sterilizer or autoclave before the test temperature is attained. On the completion of 20 minutes at the test temperature, release the steam pressure. Take the rubber pieces from the gauze and allow to cool to normal room temperature as quickly as possible. After a lapse of at least 20 minutes, but as soon after 20 minutes as possible, repeat the process successively until six heatings have been made. Complete the total cycle of six heatings within 48 hours. After the completion of the heat-treatment, keep the rubber at room temperature for at least 24 hours before subjecting it to testing for tensile strength and elongation at break (see 7.1).

7.3 Test for Tension Set — Cut out 6 mm wide parallel-sided test pieces from the palm and back portion of a pair of gloves. Make two gauge marks 50 mm apart on them. Stretch the test pieces to a length of 175 mm between gauge marks for Type A and Type C gloves and to a length of 200 mm between gauge marks for Type B for 10 minutes. Allow them to

*Methods of test for vulcanized rubbers: Part I Tensile stress-strain properties.

recover for 10 minutes, note the change in length between the gauge marks and express the change as a percentage of original distance between the gauge marks.

7.4 Reaction to Aqueous Extract — Weigh 10 g of a sample of small pieces of 3 mm². Put it into a chemically-resistant glass flask. Add 300 ml of distilled water conforming to IS: 1070-1960*. Fit the flask with a water-cooled reflex condenser with ground glass connections. Heat the water to boiling point and continue boiling for half an hour. Detach the flask from the condenser and cover immediately to prevent any possible contamination and cool the contents to $27^{\circ} \pm 2^{\circ}\text{C}$. Note the reaction of aqueous extract to one or two drops of methyl orange and phenolphthalein indicator solutions (see IS : 2263-1963†).

APPENDIX A

(Clause 6.1)

SAMPLING OF POST-MORTEM RUBBER GLOVES

A-1. SCALE OF SAMPLING

A-1.1 Lot — All the post-mortem gloves of the same type and size produced from a single mix of raw materials and processed exactly under identical conditions shall be grouped to constitute a lot.

A-1.2 Each lot shall be examined separately for judging its conformity to the requirements of this specification. For this purpose, a number of gloves shall be selected at random from the lot. The number of gloves to be selected shall depend on the size of the lot and shall be in accordance with col 1 and 2 of Table 3.

TABLE 3 SCALE OF SAMPLING

No. of GLOVES IN THE LOT	No. of GLOVES TO BE SELECTED	PERMISSIBLE No. OF DEFECTIVES FOR REQUIREMENTS OTHER THAN THOSE GIVEN IN 3.6	No. of GLOVES FOR PHYSICAL PROPERTIES OF RUBBER GIVEN IN 3.6
<i>N</i>	<i>n</i>	(3)	(4)
(1)	(2)		
2 to 5	All	0	1
6 „ 15	5	0	1
16 „ 25	6	0	1
26 „ 50	13	0	2
51 „ 100	20	0	2
101 „ 300	32	1	2
301 „ 1 000	50	2	3
1 001 and above	80	3	5

*Specification for water, distilled quality (revised).

†Methods of preparation of indicator solutions for volumetric analysis.

A-1.3 The gloves shall be selected from the lot at random. In order to ensure randomness of selection, random number tables shall be used. In case random number tables are not available, the following procedure may be adopted:

Starting from any item in the lot, count them in one order as 1, 2, 3,....., up to r and so on, where r is the integral part of N/n , N being the number of items in the lot and n the number of items to be selected. Every r th item thus counted shall be withdrawn to constitute the sample.

A-2. NUMBER OF TESTS AND CRITERIA FOR CONFORMITY

A-2.1 All the gloves selected in A-1.2 shall be examined for all the requirements of this specification except those specified for physical properties of rubber in 3.6. Any glove failing in one or more of these requirements shall be considered as defective. The lot shall be regarded as satisfactory in respect of these requirements if the number of defectives does not exceed the corresponding number given in col 3 of Table 3.

A-2.2 If the lot has been found satisfactory in A-2.1 it will be subjected to tests for requirements given in 3.6 and Table 2. The number to be tested for this purpose shall be in accordance with col 4 of Table 3 and shall be taken at random from those already selected from the lot. If none of these gloves fails in any of the requirements prescribed in 3.6 and Table 2 the lot shall be declared to have met the requirements of this specification.

BUREAU OF INDIAN STANDARDS

Headquarters:

Manak Bhavan, 9 Bahadur Shah Zafar Marg, NEW DELHI 110002

Telephones: 331 01 31, 331 13 75

Telegrams: Manaksanstha
(Common to all Offices)

Regional Offices:

	Telephone
Central : Manak Bhavan, 9 Bahadur Shah Zafar Marg, NEW DELHI 110002	{ 331 01 31 331 13 75
*Eastern : 1/14 C. I. T. Scheme VII M, V. I. P. Road, Maniktola, CALCUTTA 700054	36 24 99
Northern : SCO 445-446, Sector 35-C, CHANDIGARH 160036	{ 2 18 43 3 16 41
Southern : C. I. T. Campus, MADRAS 600113	{ 41 24 42 41 25 19 41 29 16
†Western : Manakalaya, E9 MIDC, Marol, Andheri (East), BOMBAY 400093	6 32 92 95

Branch Offices:

'Pushpak', Nurmohamed Shaikh Marg, Khanpur, AHMADABAD 380001	{ 2 63 48 2 63 49
†Peenya Industrial Area 1st Stage, Bangalore Tumkur Road BANGALORE 560058	{ 38 49 55 38 49 56
Gangotri Complex, 5th Floor, Bhadbhada Road, T. T. Nagar, BHOPAL 462003	6 67 16
Plot No. 82/83, Lewis Road, BHUBANESHWAR 751002	5 36 27
53/5, Ward No. 29, R.G. Barua Road, 5th Byelane, GUWAHATI 781003	3 31 77
5-8-56C L. N. Gupta Marg (Nampally Station Road), HYDERABAD 500001	23 10 83
R14 Yudhister Marg, C Scheme, JAIPUR 302005	{ 6 34 71 6 98 32
117/418 B Sarvodaya Nagar, KANPUR 208005	{ 21 68 76 21 82 92
Patliputra Industrial Estate, PATNA 800013	6 23 05
T.C. No. 14/1421, University P.O., Palayam TRIVANDRUM 695035	{ 6 21 04 6 21 17

Inspection Offices (With Sale Point):

Pushpanjali, First Floor, 205-A West High Court Road, Shankar Nagar Square, NAGPUR 440010	2 51 71
Institution of Engineers (India) Building, 1332 Shivaji Nagar, PUNE 411005	5 24 35

*Sales Office in Calcutta is at 5 Chowringhee Approach, P. O. Princep Street, Calcutta 700072

†Sales Office in Bombay is at Novelty Chambers, Grant Road, 89 65 28 Bombay 400007

†Sales Office in Bangalore is at Unity Building, Narasimharaja Square, 22 36 71 Bangalore 560002